



MISSOURI DEPARTMENT OF HEALTH AND SENIOR SERVICES  
 STATE PUBLIC HEALTH LABORATORY  
 BREATH ALCOHOL PROGRAM  
**DATAMASTER MAINTENANCE REPORT**

**RECEIVED**  
 By Carol Day at 10:49 am, Mar 20, 2013

REPORT #6

Complete this report at the time of the regular monthly preventive maintenance check (not to exceed 36 days).  
 Complete this report whenever the instrument is serviced or repaired and whenever it is placed into service.  
 Retain the original and send a copy within 15 days to the Breath Alcohol Program, DHSS.

DATAMASTER # 201243	NAME OF AGENCY West Plains Police Department	DATE OF INSPECTION 03/13/2013
LOCATION OF INSTRUMENT (ADDRESS AND CITY) 1912 Holiday Lane, West Plains, MO. 65775		FILE OF INSPECTION 1146

**CHECKLIST:** Place a mark in the box by each item if found to be satisfactory or if operating within established limits. (Write in observed values where determ. nec.) Unmarked items must be corrected before using instrument.

<input checked="" type="checkbox"/> DIAGNOSTIC CHECK (PRINTOUT ATTACHED)	DATE AND TIME (from printout) 03/13/2013 1146
<input checked="" type="checkbox"/> COMPUTER	<input checked="" type="checkbox"/> DETECTOR
<input checked="" type="checkbox"/> PROGRAM	<input checked="" type="checkbox"/> FILTERS
<input checked="" type="checkbox"/> HEATERS SAMPLE CHAMBER 49 °C	<input checked="" type="checkbox"/> QUARTZ STANDARD
<input checked="" type="checkbox"/> FLOW DETECTOR	<input checked="" type="checkbox"/> CALIBRATION
<input checked="" type="checkbox"/> PUMP HIGH SPEED	<input checked="" type="checkbox"/> PRINTER

<input checked="" type="checkbox"/> INDICATOR LIGHTS
<input checked="" type="checkbox"/> SIMULATOR SOLUTION SUPPLIER Repco Marketing LOT # 12001 EXP. DATE 04/02/2014
<input checked="" type="checkbox"/> SIMULATOR TEMP (34°C = 0.2°C) 34.0 °C SIMULATOR SN DR5380 EXP. DATE

CALIBRATION CHECK - (ONLY ONE STANDARD IS TO BE USED PER MAINTENANCE REPORT)

Run three tests using a standard solution. All three tests must be within ±5% of the standard value and must have a spread of .005 or less. Mark the box corresponding to the standard solution being used. (PRINTOUT ATTACHED)

<input checked="" type="checkbox"/> 0.100% STANDARD - MUST READ BETWEEN 0.095% AND 0.105% INCLUSIVE
<input type="checkbox"/> 0.080% STANDARD - MUST READ BETWEEN 0.076% AND 0.084% INCLUSIVE
<input type="checkbox"/> 0.040% STANDARD - MUST READ BETWEEN 0.038% AND 0.042% INCLUSIVE

TEST 1 • 099	TEST 2 • 100	TEST 3 • 101
--------------	--------------	--------------

PERFORM R.F.I. TEST (PRINTOUT ATTACHED)

INDICATE THE NUMBER OF BREATH TESTS IN THE FOLLOWING RANGES SINCE THE LAST MAINTENANCE REPORT:  
 (DO NOT INCLUDE SELF-ADMINISTERED TESTS)

REFUSALS 0	(0-.04) 0	(.05-.09) 2	(.10-.14) 1	(.15-.19) 0	OVER .19 1
------------	-----------	-------------	-------------	-------------	------------

LIST ANY NEW PARTS AND DESCRIBE ANY ALTERATION OR MODIFICATION THAT WAS MADE TO RESTORE THE INSTRUMENT TO OPERATE SATISFACTORILY AND WITHIN ESTABLISHED LIMITS (USE OTHER SIDE IF NECESSARY).

<b>INSPECTING OFFICER</b>	
SIGNATURE <i>[Signature]</i>	PRINT NAME Brandon Romans
TYPE (PRINT) NUMBER/EXPIRATION DATE 210063 / 05-16-2013	TELEPHONE NUMBER (417) 256-2244

RETURN COMPLETED REPORT TO THE: Breath Alcohol Program, MO Department of Health and Senior Services, Southeast District Office, 2875 James Blvd., Poplar Bluff, MO 63901

**CERTIFICATE OF ANALYSIS**

**MANUFACTURER AND SUPPLIER:** RepCo Marketing, Inc.

**LOT NUMBER:** 12001

**EXPIRATION DATE:** April 2, 2014 at 11:59 p.m.

RepCo Marketing, Inc. certifies the following:

RepCo Marketing, Inc. manufactured, tested and supplied Lot Number 12001 of Alcohol Certified Solution for simulators. Random samples of said lot number were analyzed by an independent laboratory utilizing a gas chromatograph and found to contain .1205 gms/dl +/- .003 gms/dl wt/vol ethanol (95% Confidence).

The alcohol and distilled water used in the solution were found to be free of any interfering substance.

This solution will produce a vapor alcohol value of .100 +/-3% gms/210L Breath when heated to 34 Degrees Celsius +/-0.2 Degrees Celsius in a simulator (95% Confidence).

The date of manufacture for this lot number is April 3, 2012. The expiration date for this lot number is April 2, 2014 at 11:59 p.m.

This document is a true representation of the original Certificate of Analysis.



Cecil B. Garner, President  
RepCo Marketing, Inc.



Face This Side Down - This Edge In First

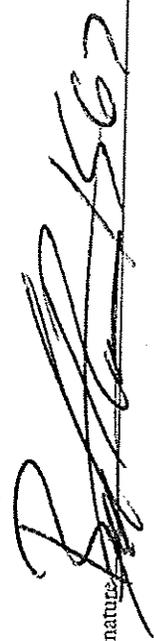
**BAC DataMaster  
Evidence Ticket**

STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT  
BAC DATAMASTER SERIAL NUMBER 991849  
09/13/19

ARREST TIME: 11:30  
SUBJECT NAME:  
RT/TEST  
DOB: 09/17/79 SEX: M  
STATE ID.: MW089879  
ARRESTING OFFICER:  
ROMANS/BRANTON  
OFFICER I.D.: 567  
TESTING OFFICER:  
ROMANS/BRANTON  
OFFICER I.D.: 567  
PERMIT NUMBER: 21886  
EXPIRATION DATE: 05/15/19  
MISCELLANEOUS DATA:  
021 YEST

--- BREATH ANALYSIS ---

BLANK TEST .000 11:57  
INTERNAL STANDARD USE1078 11:57  
RATIO INTERFERENCE

Operator Signature: 

Face This Side Down - This Edge In First

**BAC DataMaster  
Evidence Ticket**

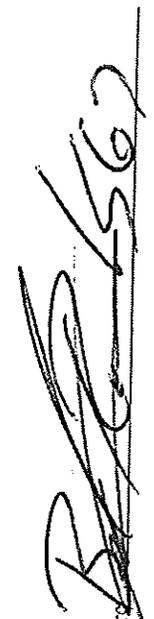
STATE OF MISSOURI  
WEST PLAINS POLICE DEPARTMENT  
BAC DATAMASTER SERIAL NUMBER 991849  
09/13/19

ARREST TIME: 11:30  
SUBJECT NAME:  
TEST  
DOB: 09/17/79 SEX: M  
STATE ID.: MW089879  
ARRESTING OFFICER:  
ROMANS/BRANTON  
OFFICER I.D.: 567  
TESTING OFFICER:  
ROMANS/BRANTON  
OFFICER I.D.: 567  
PERMIT NUMBER: 21886  
EXPIRATION DATE: 05/15/19  
MISCELLANEOUS DATA:  
TEST

--- BREATH ANALYSIS ---

BLANK TEST .000 11:59  
INTERNAL STANDARD USE1078 11:59  
SUBJECT SAMPLE .000 11:59  
BLANK TEST .000 11:59

4 Seconds

Operator Signature: 

State of Missouri  
DEPARTMENT OF HEALTH



P E R M I T  
TYPE II



BRANDON ROMANS

is hereby authorized to instruct and supervise operators, train instructors, inspect, calibrate, perform field repairs, and operate the following breath analyzer(s):

DATAMASTER

for the determination of the alcoholic content of blood from a sample of expired (alveolar) air, issued under the provisions of sections 577.020 through 577.041, RSMo 1988.

Date 05/16/2011

Number 210063

Expires 05/16/2013

Director of State Public Health Laboratory

Director, Department of Health